
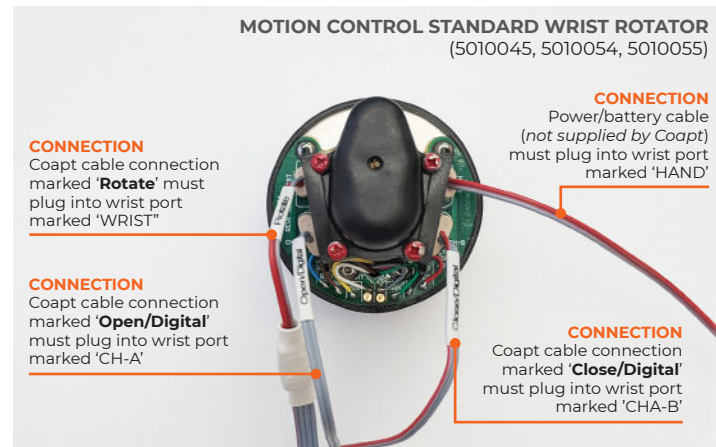


17

CLINICAL CONNECTIONS & SETTINGS GUIDE

17 controls pronation/supination of powered wrists and direct pattern recognition command of the new generation Ottobock bebionic. (*with serial numbers BB1000-0_B)*

PART 1: PHYSICAL CONNECTIONS

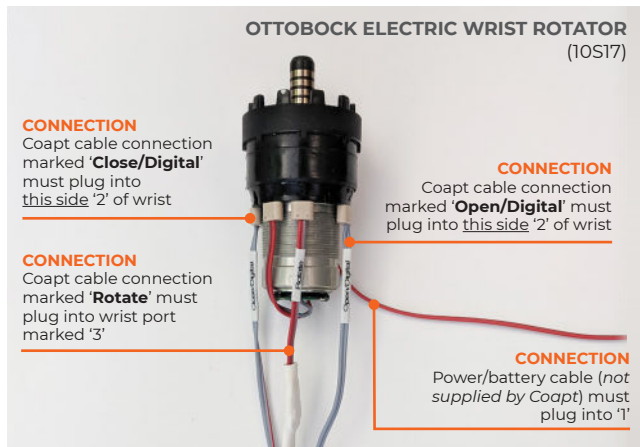

PART 2: SOFTWARE SETTINGS

ELBOW

ESPIRE CLASSIC PLUS

For more information on connecting our Coapt System to this device please reference our Espire Classic Plus + Coapt Compatibilites Guide.



WRISTS

OTTOBOCK ELECTRIC WRIST ROTATOR (NO MYOROTRONIC)

No settings required

MOTION CONTROL STANDARD WRIST ROTATOR (NO PROCONTROL)

No settings required

HANDS

OTTOBOCK BEBIONIC*

Ensure hand settings are the factory defaults