


HO

CLINICAL CONNECTIONS & SETTINGS GUIDE

HO controls open/close operation of prosthetic hands where no powered wrist or elbow is present. Pattern recognition command of multifunction grips is not included.

PART 1: PHYSICAL CONNECTIONS

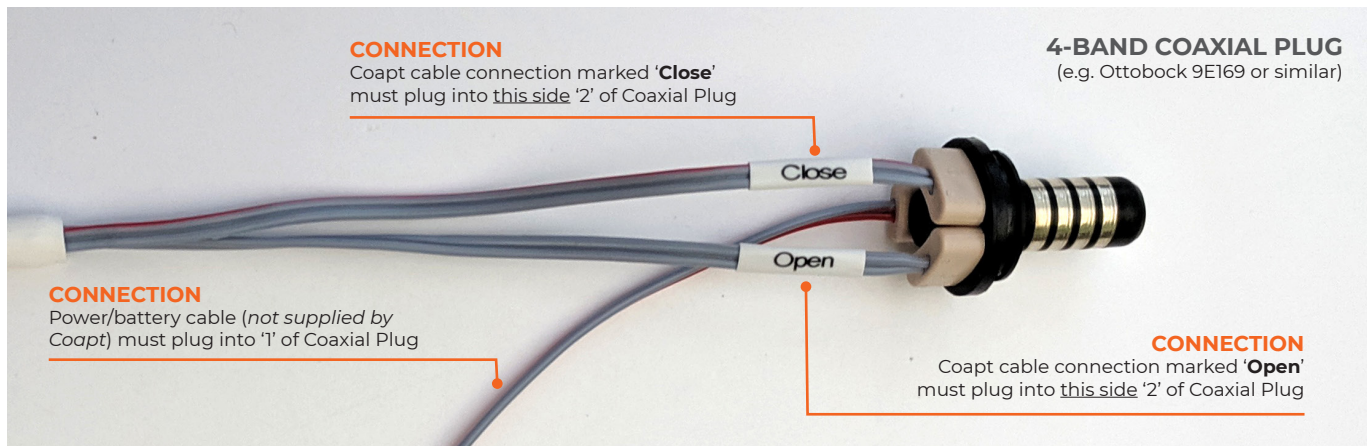

PART 2: SOFTWARE SETTINGS

HANDS

I-LIMB, TASKA, VINCENTEVOLUTION3, PSYONIC ABILITY HAND, COVVI HAND

Ensure hand settings are the factory defaults

OTTOBOCK SENSORHAND, MYOHAND VARIPLUS, SYSTEM ELECTRIC GREIFER, OR SYSTEM ELECTRIC HAND

Ensure 'control mode'/'program' 1

OTTOBOCK BEBIONIC

Control Strategy: Dual Site

Open / Close Strategy: Electrodes: A,B

Control Options: Electrodes

Control Response: Proportional

In ELECTRODE SCREEN:

- Channel 1 "Blue" threshold: 10%, Channel 1 "Red" threshold: 90%, Channel 2 "Blue" threshold: 10%, Channel 2 "Red" threshold: 90%

Remember to press "Send to Hand" after making any changes

MOTION CONTROL PROHAND, PROETD/ETD2

HAND SET UP

- Input Type: EMG, Hand Filtering: Quick, Channel: Dual, Conatrol: Differential, Hand Direction: A

Thresholds/Outputs

- A: 15, B: 15

Input Gains

- A: 5, B: 5