


HO CLINICAL CONNECTIONS & SETTINGS GUIDE

HO controls open/close operation of prosthetic hands where no powered wrist or elbow is present. Pattern recognition command of multifunction grips is not included.

PART 1: PHYSICAL CONNECTIONS

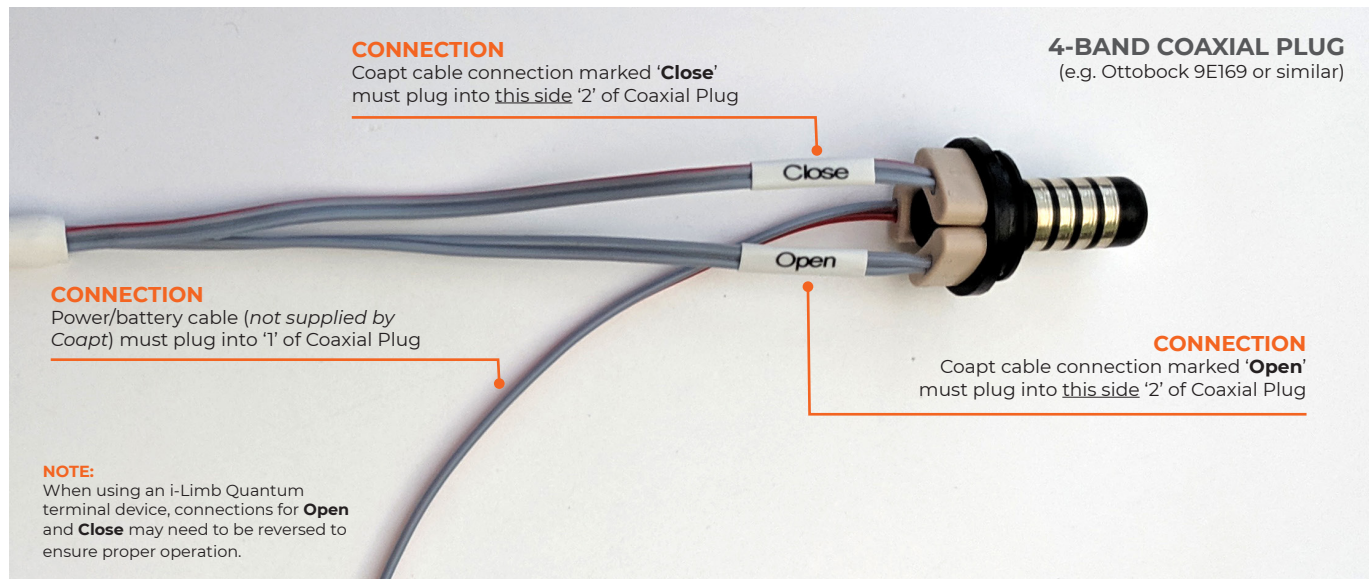

PART 2: SOFTWARE SETTINGS

ELBOW

ESPIRE CLASSIC PLUS

For more information on connecting our Coapt System to this device please reference our Espire Classic Plus + Coapt Compatibilites Guide.



HANDS

*****MANY/MOST HANDS SHOULD BE SET TO FACTORY DEFAULT FOR OPTIMAL OPERATION.**

OTTOBOCK SENSORHAND, MYOHAND VARIPLUS, SYSTEM ELECTRIC GREIFER, OR SYSTEM ELECTRIC HAND

Ensure 'control mode'/'program' 1

OTTOBOCK BEBIONIC

Control Strategy: Dual Site

Open / Close Strategy: Electrodes: A,B

Control Options: Electrodes

Control Response: Proportional

In ELECTRODE SCREEN:

- Channel 1 "Blue" threshold: 10%, Channel 1 "Red" threshold: 90%, Channel 2 "Blue" threshold: 10%, Channel 2 "Red" threshold: 90%

Remember to press "Send to Hand" after making any changes

MOTION CONTROL PROHAND, PROETD/ETD2

HAND SET UP

- Input Type: EMG, Hand Filtering: Quick, Channel: Dual, Conatrol: Differential, Hand Direction: A

Thresholds/Outputs

- A: 15, B: 15

Input Gains

- A: 5, B: 5

PSYONIC ABILITY HAND

Ensure the "Control System" setting in the PSYONIC ABILITY HAND app is set to "Direct Control"

Ensure all other hand settings in the PSYONIC ABILITY HAND app are set to the factory defaults

ADAMS HAND

Ensure the "Control System" setting in the Adam's Hand is set to "Coapt"