
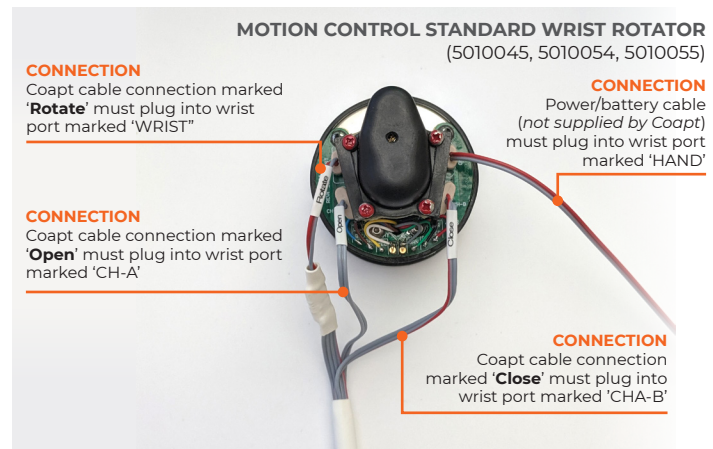


15

# CLINICAL CONNECTIONS & SETTINGS GUIDE

15 controls pronation/supination of powered wrists and operation of Motion Control powered wrist flexion/extension with ProHand or ProETD/ETD2 open/close.

## PART 1: PHYSICAL CONNECTIONS

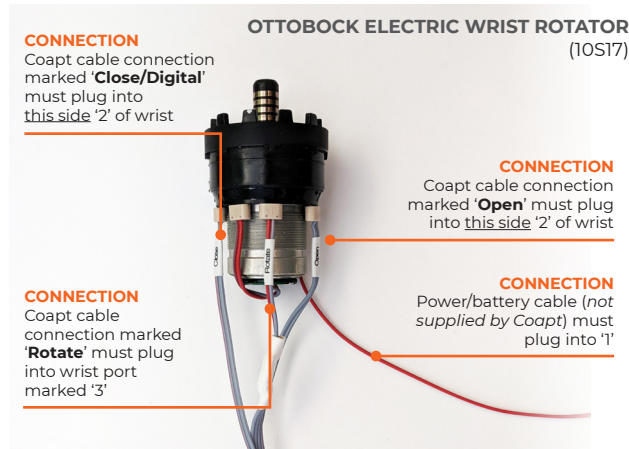

### WRISTS

#### MOTION CONTROL POWERED FLEXION WRIST

Wrist Direction: A

#### RELAX DELAY

- Relax Timer: 0.1

#### SWITCH CONTROL

- Switch Rates A: 75
- Switch Rates B: 75
- Switch Window: 0.1
- Fast Access: On
- Co-Contraction: Off
- Auto-Switch Back: No

#### POWERED FLEXION WRIST SETTINGS

- Motor Speed: High
- Motor Brake: On
- Home Position Delay: 0.5

#### OTTOBOCK ELECTRIC WRIST ROTATOR (NO MYOROTRONIC)

No settings required

#### MOTION CONTROL STANDARD WRIST ROTATOR (NO PROCONTROL)

No settings required

### HANDS

#### MOTION CONTROL PROHAND, PROETD/ETD2

##### HAND SET UP

- Input Type: EMG
- Hand Filtering: Quick
- Channel: Dual
- Control: Differential
- Hand Direction: A

##### Thresholds/Outputs

- A: 15
- B: 15

##### Input Gains

- A: 5
- B: 5