


16

CLINICAL CONNECTIONS & SETTINGS GUIDE

16 allows pattern recognition command of Ottobock Michelangelo Hand or AxonHook with optional Ottobock AxonRotation.

PART 1: PHYSICAL CONNECTIONS

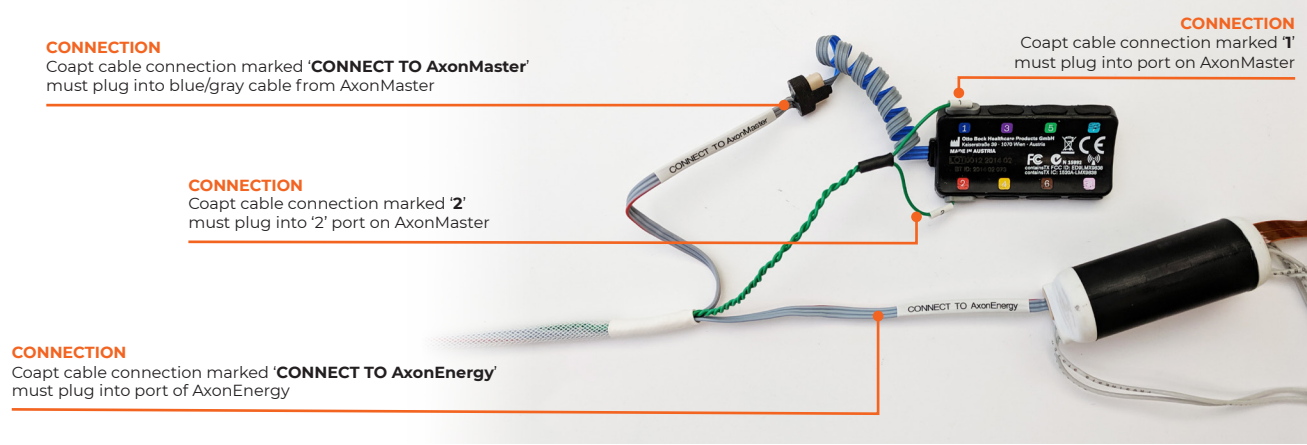

PART 2: SOFTWARE SETTINGS

WRISTS

OTTOBOCK AXONROTATION (OPTIONAL)

Ensure all settings in the Ottobock Data Station 'Customizing' screen are set exactly as shown.

HANDS

OTTOBOCK MICHELANGELO HAND, AXONHOOK

Ensure all settings in the Ottobock Data Station 'Customizing' screen are set exactly as shown.

